Product information

ATEC Drill

ø 1.0 mm / Endoseal

REF: O.27.28.B044.051 (Length 21 mm)

O.27.28.B044.052 (Length 28 mm)



StecoGuide Endo-Sleeve

for ATEC Drill

REF: M.27.28.D100L5



System expansion

Further drilling steps by StecoGuide outer sleeve and inner sleeves in different diameters are possible.



Further products

StecoGuide

Precise implant planning:
Drill sleeves for every case



Magnetic extrusion


For decapitated teeth:
carefully crown-lengthening



Titanmagnetics®

Magnetic attachments for implants:
Secure prosthesis retention

- secure prosthesis hold
- easy handling
- no matrix change



Please contact us at info@steco.de

steco-system-technik GmbH & Co. KG
Kollaustr. 6 • 22529 Hamburg • Germany
Tel. +49 40 55 77 81-0• www.steco.de/en

K.27.14.EN03 (03.2025)

steco system-technik

GuidedEndo

Template-guided Endodontics.
Simply guiding!

StecoGuide

Obliterated - Calcified Teeth

3D Planning

Opening an opliterated root canal can be difficult, as it cannot be controlled visually.

With a 3D planning software the drilling axis is defined (e.g. with coDiagnostiX™ or other systems).

Drill and sleeve geometry can be integrated in the software.

StecoGuide Endo-Sleeve

Drill- and sleeve-geometry are positioned in the desited axis in the software and can be inserted into a milled or printed the drill sleeve surgical template.

Guided root axis processing

Sleeve-guided canal openening treatment offers predictable safety.

- time-saving
- tissue preserving
- lower risk of perforation

The ATEC twist drill is precisely guided by the StecoGuide Endo-Sleeve.







For more information, visit www.steco.de/en

Photos: University Centre for Dental Medicine Basel (Krastl, Connert, Kühl) and coDiagnostiX™

Produktinformation

ATEC-Bohrer

ø 1,0 mm / Endoseal

REF: O.27.28.B044.051 (Länge 21 mm)

O.27.28.B044.052 (Länge 28 mm)



StecoGuide Endo-Hülse

für ATEC-Bohrer geeignet

REF: M.27.28.D100L5



Systemerweiterung

Weitere Bohrschritte durch StecoGuide Außen- und Innenhülsen in verschiedenen Durchmessern möglich.



Weitere Produkte

StecoGuide

Präzise Implantatplanung:
Bohrhülsen für jeden Fall



Magnetische Extrusion

Bei dekapierten Zähnen:
schonende Kronenverlängerung



Titanmagnetics®

Magnetattachments für Implantate:

- sicherer Prothesenhalt
- leichtes Handling
- kein Matrizenwechsel




Rufen Sie uns gerne an!
Telefon +49 40 - 55 77 81-0

steco-system-technik GmbH & Co. KG
Kollaustr. 6 • 22529 Hamburg • Deutschland
E-Mail: info@steco.de • www.steco.de


K.27.14.DE02 (03.2025)

steco system-technik

GuidedEndo

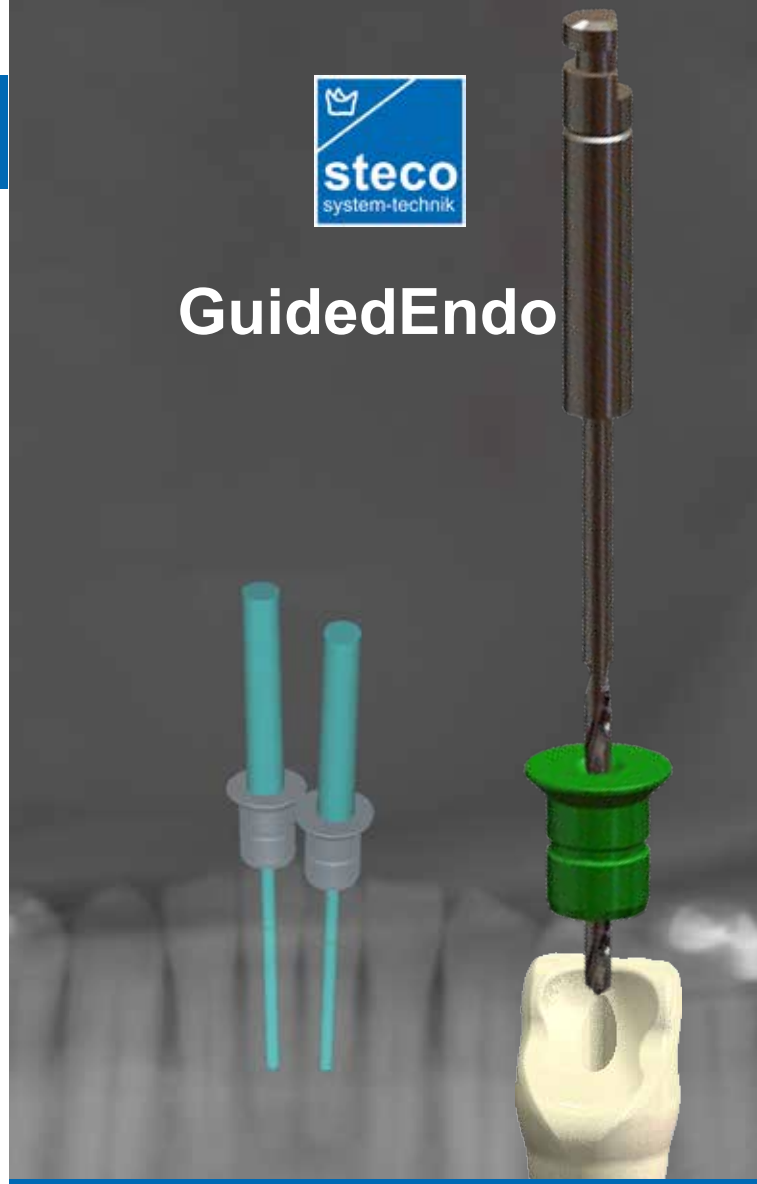

Schablonengeführte Endodontie.
Einfach führend!

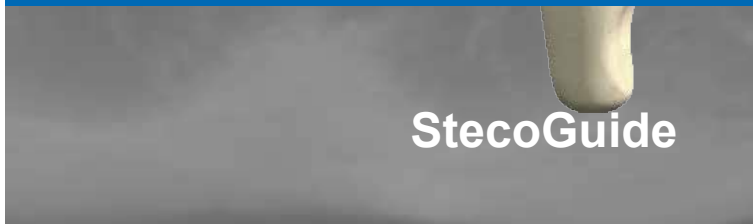

StecoGuide

Obliterierte - kalzifizierte Zähne

3D-Planung

Die Eröffnung eines opliterierten Wurzelkanals kann schwierig sein, da sie optisch nicht kontrollierbar ist.

Mit einer 3D-Planungssoftware wird der Bohrkanal festgelegt (z. B. mit coDiagnostiX™ oder anderen Systemen).

Bohrer- und Hülsengeometrie lassen sich in der Software integrieren.

StecoGuide Endo-Hülse

Die Titanhülse wird virtuell in der Planungssoftware positioniert und anschließend in eine gefräste oder gedruckte Bohrschablone gesteckt.

Geführte Wurzelkanalaufbereitung

Die hülsengeführte Kanalaufbereitung bietet planbare Sicherheit.

- zeitsparend
- substanzschonend
- geringere Perforationsrisiken

Der ATEC-Spiralbohrer wird durch die StecoGuide Endo-Hülse präzise geführt.







Weitere Informationen unter
www.steco.de

Fotos: Universitäres Zentrum für Zahnmedizin Basel (Krastl, Connert, Kühl) und coDiagnostiX™